

Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

Optical Fiber Diameter Analyser (OFDA 100) Micron Test Report

Alpakas vom Josefsberg/Eva Klingbacher

Josefsberg 11

9470 St. Paul Austria

Date: 06/26/18

Test No: 962484

Animal and Sample Description


Animal Name: AHN Murphey
Breed: Alpaca(Huacaya)
Sex: Male
Color: Black

Animal ID: 528210002756195
Sample Location: Mid Side
Sample Date: 06/21/18
Age: 06/07/13

Laboratory Data

Mean Fiber Diameter: 20.9 microns
Standard Deviation: 5.2 microns
Coefficient of Variation: 24.8 %
Spin Fineness: 21.1 microns

Fibers Greater Than 30 microns: 5.7 %
Comfort Factor: 94.3 %
Mean Curvature: 33.1 deg/mm
SD Curvature: 21.5 deg/mm

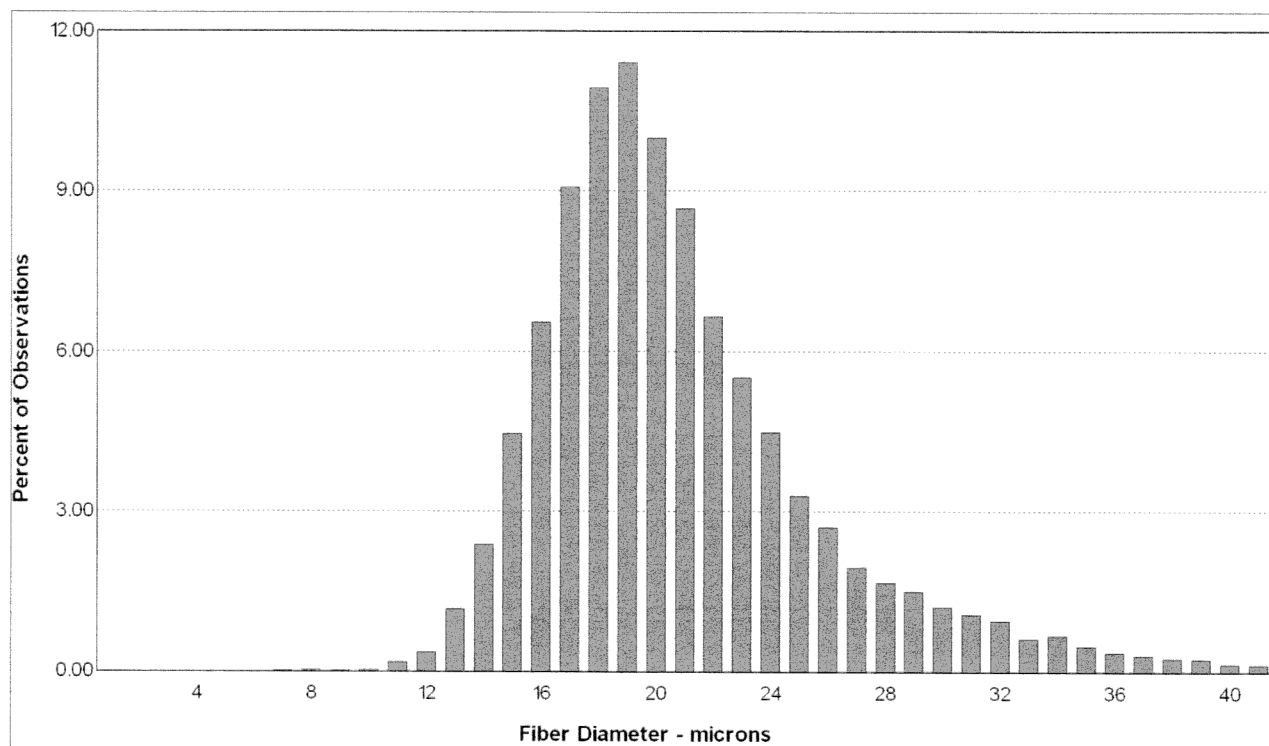

This Test Performed According to I.W.T.O Method 47